


NOTES: UNLESS OTHERWISE SPECIFIED

- SMALLER OXYGEN TANKS ARE NOT USABLE. IF USING OXYGEN GENERATOR OR CONCENTRATOR IT MUST SUPPLY AT LEAST 30 lpm @ 50 PSI (3.4 BAR)

REVISIONS			
REV	DESCRIPTION	DATE	APPROVED
-	INITIAL RELEASE	01/17/2018	WSH

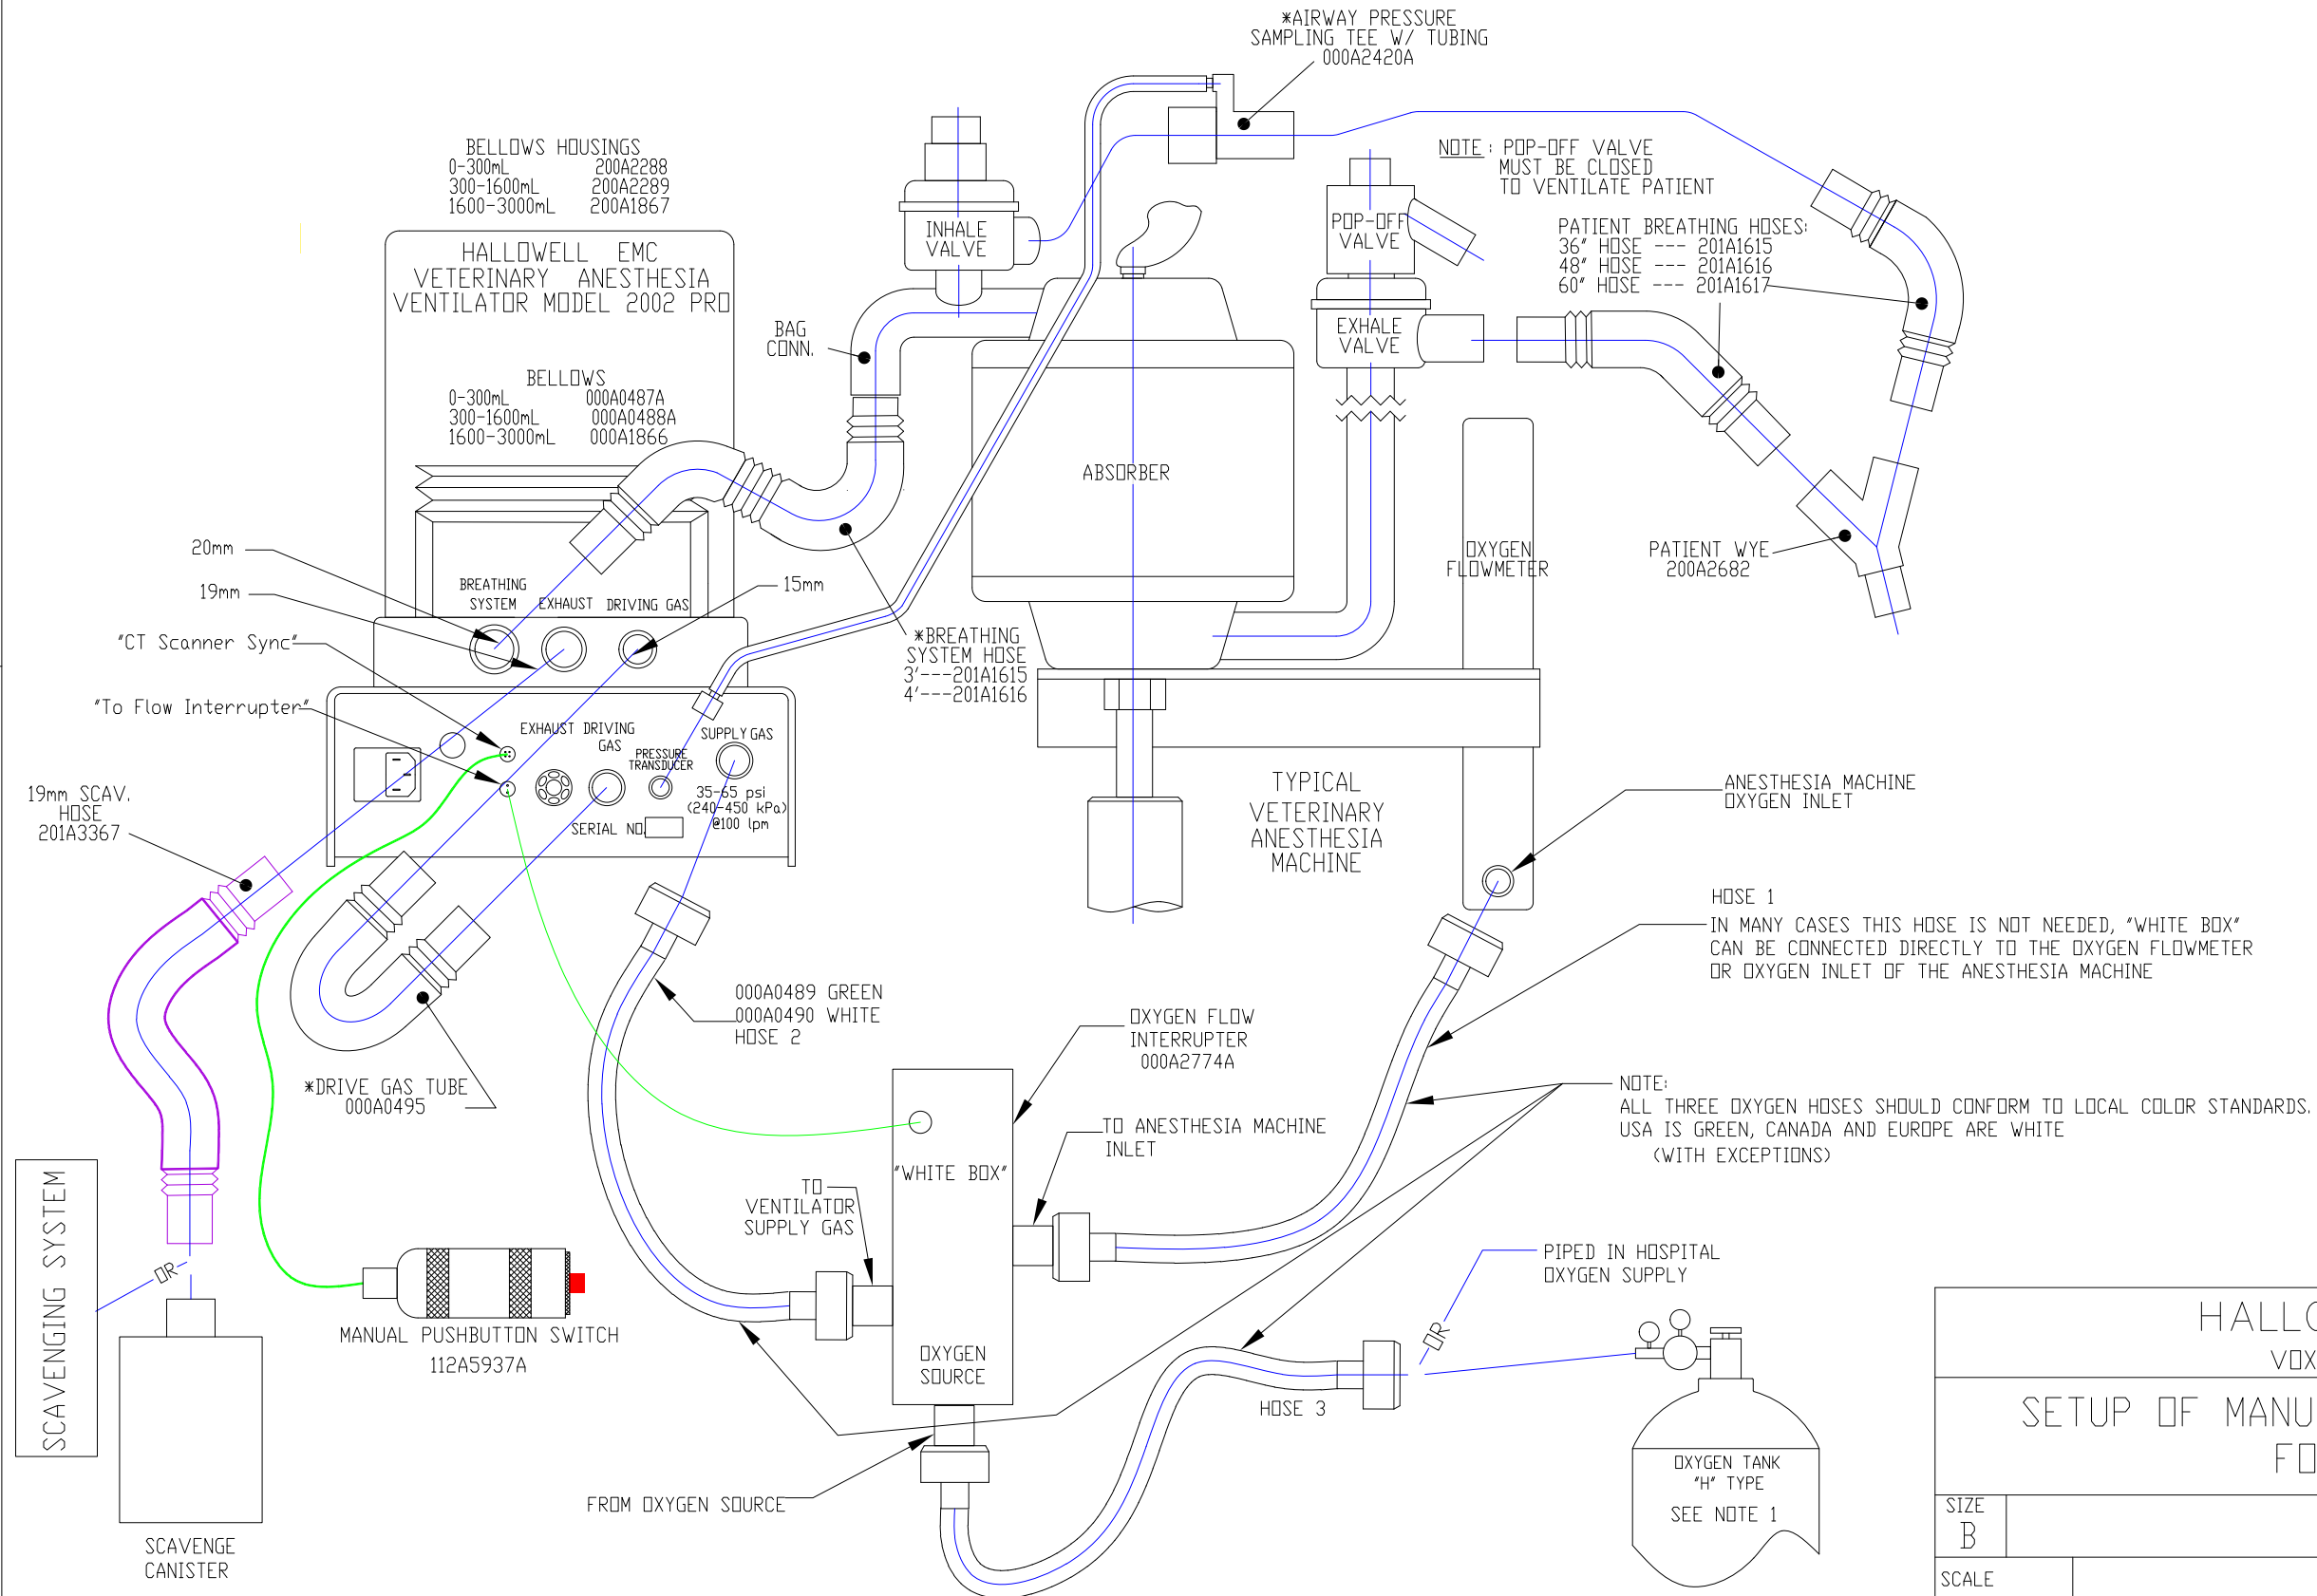

*COMPONENTS SUPPLIED WITH MODEL 2002 PRO VENTILATOR

HALLOWELL EMC
VOX: (413) 445-4263

SETUP OF MANUAL VENTILATION PAUSE FOR IMAGING

SIZE B	BLCB0329	
SCALE	SHEET	1 OF 1